

ELUXEO[®] EB-840S

STANDARD TYPE BRONCHOSCOPE




NEW




ELUXEO® EB-840S BRONCHOSCOPE - Standard Type



This standard video bronchoscope has a distal end diameter of 4.8 mm and a minimum instrument channel diameter of 2.2 mm. This allows endotherapeutic devices to pass through smoothly - for diagnostic and interventional procedures. It is compatible with EP-8000, VP-7000 and EP-6000 processors. The One-Step Connector can be connected easily to the light source in a single step. The EB-840S is compatible with low temperature plasma sterilisation.

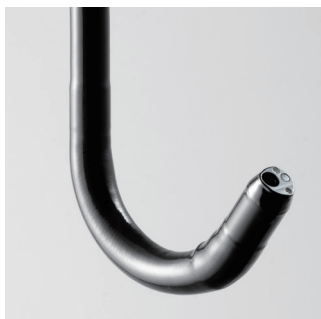

Field of view	120°
Observation range	2-100 mm
Bending capability	Up 210° / Down 130°
Ø Distal end	4.8 mm
Ø Insertion tube	5.1 mm
Min. Ø instrument channel	2.2 mm
Working length	600 mm
Total length	880 mm
Compatible Processors/ Light Source	EP-8000, VP-7000/BL-7000, EP-6000
Sterilisation	STERRAD®* /EOG
Compatible with low temperature plasma sterilisation.	

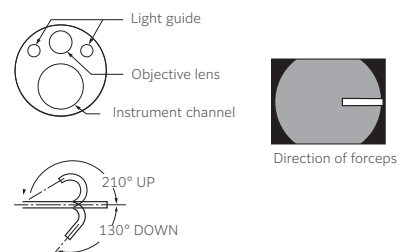


EB-580S + VP-7000



EB-840S + VP-7000

HD image sensor with large visual view for operator


The CMOS video sensor produces HD images in the wider size which supports diagnosis

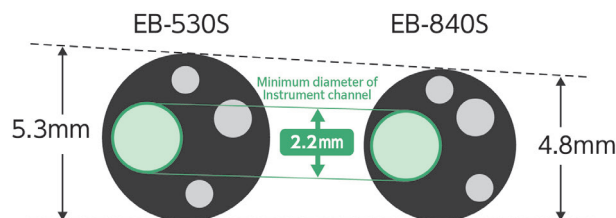

4.8 mm distal end diameter

2.2 mm minimum diameter of instrument channel

Maintaining the previous suction performance, the tip diameter was slimmed to improve bronchi insertion.

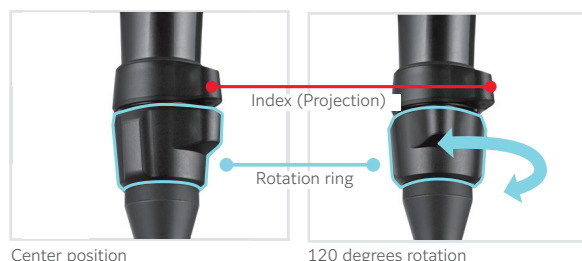

Rotation function

Rotation function enables 120 degrees rotation of the insertion portion.



Enhanced control portion with improved ergonomics

Control portion equipped with a wider grip, suction valve, and four switches.

FUJIFILM

Manufactured and distributed by
FUJIFILM Corporation
26-30, Nishiazabu 2-chome, Minato-ku,
Tokyo 106-8620, JAPAN
www.fujifilm.com

Authorised Representative
FUJIFILM Healthcare Europe GmbH
Balcke-Dürr-Allee 6, 40882 Ratingen,
Germany

Importer
FUJIFILM Europe B.V.

© 2026 FUJIFILM Healthcare Europe GmbH

Specifications are subject to change without notice. All brand names or trademarks are the property of their respective owners. In some countries, regulatory approval may be required to import medical devices. For proper use of the products, be sure to read the instruction for use prior to use. For the availability of these products, please contact your local sales representatives.